

Configuration: Asset Sub Types



This guide offers a straightforward approach to managing asset subtypes, making it essential for anyone looking to streamline their asset management process. It covers creating, editing, and deleting subtypes with clear, step-by-step instructions, ensuring users can efficiently customize their asset categories. By following this guide, users can enhance organization, improve data accuracy, and better manage their assets, making it a valuable resource for effective asset management.

Creating Asset Sub Types

1

In this guide we will demonstrate how to create and configure asset subtypes. Click on a configuration menu.

The screenshot shows the MicadPro Asset Register interface. The left sidebar has a 'Configuration' menu item highlighted with a yellow circle. The main area displays a table of assets with the following columns: ID, DESCRIPTION, STATUS, TYPE, SUB TYPE, and REGION. The table contains 14 rows of data, including fire doors and air handling units.

ID	DESCRIPTION	STATUS	TYPE	SUB TYPE	REGION
4	Fire Door - 00004	Broken	Fire Doors	ANAESTHETICS GEN EQUIP	C..TestRegionLoc34
5	Fire Door - 00005	Broken	Fire Doors	BOYLES MACHINE	R..oss Hall Hospital
6	Fire Door - 00006	Broken	Air Handling Unit	DENTAL ANAESTHETIC EQUIP	R..oss Hall Hospital
7	Fire Door - 00007	Expired	Fire Doors	RESUSCITATION TROLLEY	R..oss Hall Hospital
8	Fire Door - 00008	Existing/In Use	Fire Doors	TestAV-ST	R..oss Hall Hospital
9	Fire Door - 00009	Existing/In Use	Air Handling Unit	RESUSCITATION TROLLEY	R..oss Hall Hospital
10	Fire Door - 00010	Existing/In Use	Extractor Fan	RESUSCITATION TROLLEY	R..oss Hall Hospital
11	Fire Door - 00011	Existing/In Use	Fire Door - 60min	INCUBATOR	R..oss Hall Hospital
12	Fire Door - 00012	Existing/In Use	Air Handling Unit	PULMONARY FUNCTION REC	R..oss Hall Hospital
13	Fire Door - 00013	Existing/In Use	Fire Door - 30min	BOYLES MACHINE	R..oss Hall Hospital
14	Fire Door - 00014	Existing/In Use	Fire Door - 30min	RESUSCITATION TROLLEY	R..oss Hall Hospital

2 Click on 'Edit Sub Type.'

The screenshot shows the micad pro dashboard interface. At the top, there is a navigation bar with the micad pro logo, a notification bell, and the user profile for Ian Johnson (Admin [devalpha]). Below the navigation bar, there is a grid of action buttons for various system components. The 'Asset Sub Type' button is highlighted with a yellow circle. Other buttons include 'Edit Asset Status', 'Edit Asset Type', 'Edit Model', 'Edit Supplier', 'Edit Unit', 'Edit Availabilities', 'Edit Custom Fields', and 'System Parameters'.

3 To create a new Sub Type, click 'Create Sub Type.'

The screenshot shows the 'Sub Type Configuration' table in the micad pro dashboard. The table has columns for 'ASSET TYPE', 'LIFE', 'NORMAL WARRANTY', 'MIN LIFE', 'MAX LIFE', and 'STANDARD LIFE'. A search bar is located at the top left of the table. The '+ Create Sub Type' button is highlighted with a yellow circle. The table contains the following data:

ID	ASSET TYPE	LIFE	NORMAL WARRANTY	MIN LIFE	MAX LIFE	STANDARD LIFE
ch	<input type="text" value="Search"/>	<input type="text" value=""/>				
CITATION TROLLEY	Fire Door - External	No	0	0	0	0
ANAESTHETIC EQUIP	Fire Doors	No	0	0	0	0
L ANAESTHETIC EQUIP	Fire Door - External	No	0	0	0	0
MACHINE	Fire Door - External	No	0	0	0	0
ATOR	Fire Door - External	No	0	0	0	0
IE SECONDARIES	Fire Alarms - Associated Equipment - Healthcare	No	0	0	0	0
INARY FUNCTION REC	Fire Door - External	No	0	0	0	0
THETICS GEN EQUIP	Fire Alarms - Associated Equipment - Healthcare	No	0	0	0	0
CITATOR RESPIRATRY	Fire Door - External	No	0	0	0	0
.ALARM PNEUMATIC	Fire Doors	Yes	14	17	12	13
-ST		No	0	0	0	0
-ST		No	0	0	0	0


4 First, click in 'Details' to give the new Sub Type a name.

The screenshot shows the 'Asset Sub Type Configuration' page. A modal window titled 'Create Sub Type' is open. The modal contains several input fields: 'Details *' (highlighted with a yellow circle), 'Normal Warranty', 'Asset Type' (a dropdown menu), 'Min Life', 'Life' (a toggle switch), 'Max Life', and 'Standard Life'. A 'SAVE' button is located at the bottom right of the modal. The background shows a table with columns: ID, DETAILS, ASSET TYPE, LIFE, NORMAL WARRANTY, and MIN LI.


5 Click on the asset type drop-down to link this subtype

The screenshot shows the 'Asset Sub Type Configuration' page. A modal window titled 'Create Sub Type' is open. The modal contains several input fields: 'Details *' (with 'New SubType' entered), 'Normal Warranty', 'Asset Type' (a dropdown menu highlighted with a yellow circle), 'Min Life', 'Life' (a toggle switch), 'Max Life', and 'Standard Life'. A 'SAVE' button is located at the bottom right of the modal. The background shows a table with columns: ID, DETAILS, ASSET TYPE, LIFE, NORMAL WARRANTY, MIN LIFE, and MAX.

6 with a parent asset type.

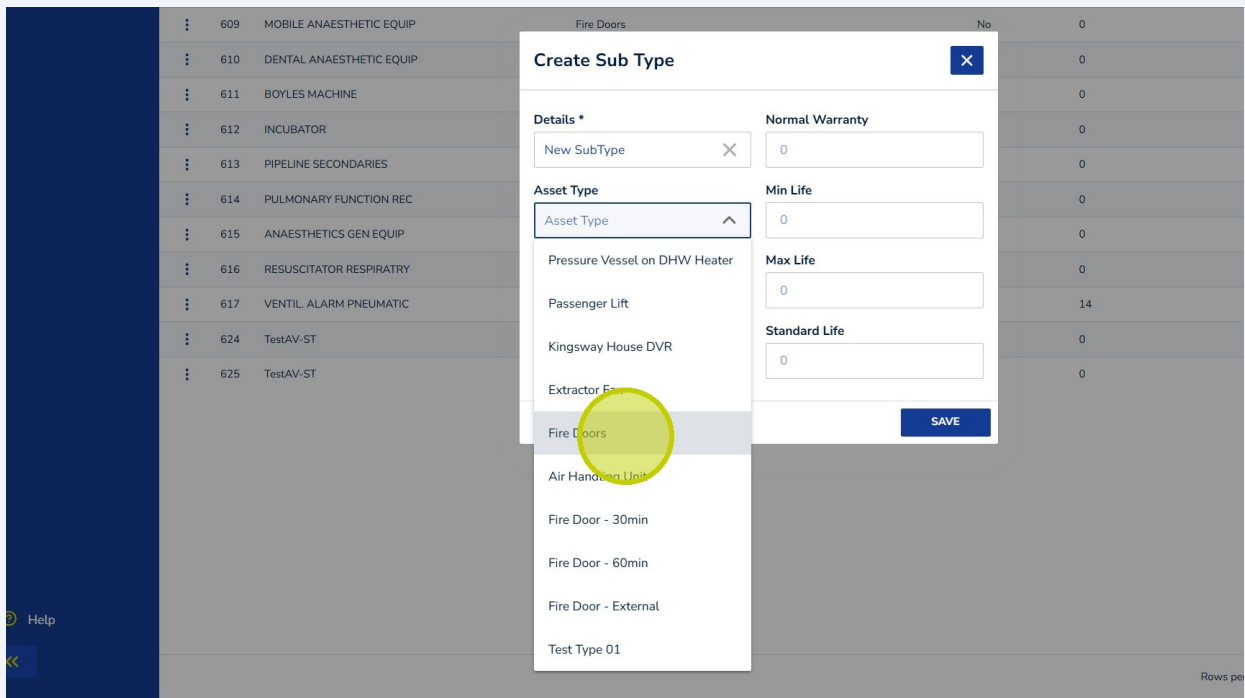

7 If required, click the life toggle to activate the fields on the right.

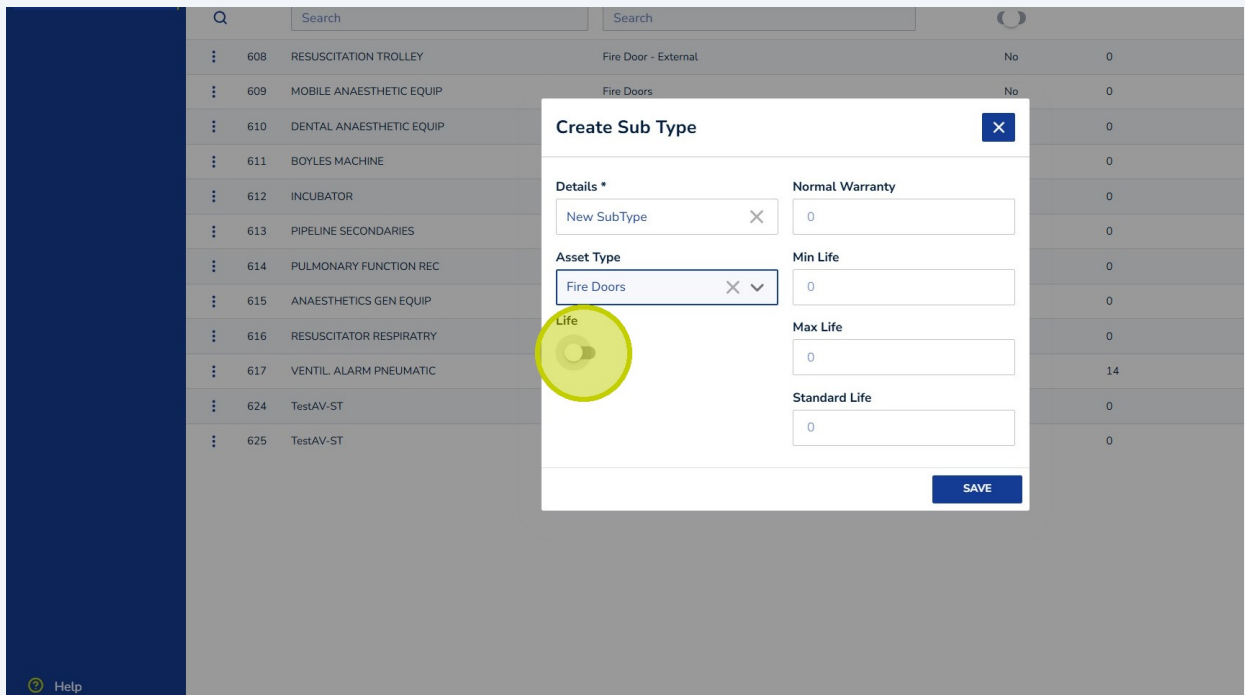

8

You can enter values in these four fields, which in a future release will self-calculate certain aspects of the asset.

The screenshot shows the 'Asset Sub Type Configuration' page in the 'micap pro' system. A modal window titled 'Create Sub Type' is open, allowing configuration for a new sub-type. The modal contains the following fields:

- Details ***: A text input field containing 'New SubType'.
- Asset Type**: A dropdown menu set to 'Fire Doors'.
- Life**: A toggle switch that is currently turned on.
- Normal Warranty**: A numeric input field with a value of 0, highlighted by a yellow circle.
- Min Life**: A numeric input field with a value of 0.
- Max Life**: A numeric input field with a value of 0.
- Standard Life**: A numeric input field with a value of 0.

A 'SAVE' button is located at the bottom right of the modal. The background shows a table with columns: ID, DETAILS, ASSET TYPE, LIFE, NORMAL WARRANTY, MIN LIFE, MAX LIFE, and STANDARD LIFE. The table contains several rows of asset data.

9

Once you have completed this form, click 'Save'.

This screenshot shows the same 'Create Sub Type' modal as in the previous image, but with the 'Normal Warranty' field now containing the value '5'. The 'SAVE' button at the bottom right of the modal is highlighted with a yellow circle, indicating the next step in the process.

10 Your new Sub Type will appear at the bottom of the table.

MOBILE ANAESTHETIC EQUIP	Fire Doors	No	0	0	0	0
DENTAL ANAESTHETIC EQUIP	Fire Door - External	No	0	0	0	0
BOYLES MACHINE	Fire Door - External	No	0	0	0	0
INCUBATOR	Fire Door - External	No	0	0	0	0
PIPELINE SECONDARIES	Fire Alarms - Associated Equipment - Healthcare	No	0	0	0	0
PULMONARY FUNCTION REC	Fire Door - External	No	0	0	0	0
ANAESTHETICS GEN EQUIP	Fire Alarms - Associated Equipment - Healthcare	No	0	0	0	0
RESUSCITATOR RESPIRATRY	Fire Door - External	No	0	0	0	0
VENTIL. ALARM PNEUMATIC	Fire Doors	Yes	14	17	12	13
TestAV-ST		No	0	0	0	0
TestAV-ST		No	0	0	0	0
New SubType	Fire Doors	Yes	5	5	5	5

Rows per page: 25 | 1 - 13 of 13 | < 1

11 You can use this table to search Sub Types, either by the Sub Type name

Current Application
Asset

Asset Register

Configuration

Asset Sub Type Configuration

ID	DETAILS	ASSET TYPE	LIFE	NORMAL WARRANTY
608	RESUSCITATION TROLLEY	Fire Door - External	No	0
609	MOBILE ANAESTHETIC EQUIP	Fire Doors	No	0
610	DENTAL ANAESTHETIC EQUIP	Fire Door - External	No	0
611	BOYLES MACHINE	Fire Door - External	No	0
612	INCUBATOR	Fire Door - External	No	0
613	PIPELINE SECONDARIES	Fire Alarms - Associated Equipment - Healthcare	No	0
614	PULMONARY FUNCTION REC	Fire Door - External	No	0
615	ANAESTHETICS GEN EQUIP	Fire Alarms - Associated Equipment - Healthcare	No	0
616	RESUSCITATOR RESPIRATRY	Fire Door - External	No	0
617	VENTIL. ALARM PNEUMATIC	Fire Doors	Yes	14
624	TestAV-ST		No	0
625	TestAV-ST		No	0
626	New SubType	Fire Doors	Yes	5

12 Cor the asset type name.

The screenshot shows the 'Asset Sub Type Configuration' page in the micadpro application. The page has a blue sidebar on the left with 'Asset Register' and 'Configuration' options. The main content area has a header with the micadpro logo and 'Current Application Asset'. Below the header is a table with columns: ID, DETAILS, ASSET TYPE, LIFE, NORMAL WARRANTY, and MIN. The table contains one row with ID 626, DETAILS 'New SubType', ASSET TYPE 'Fire Doors', LIFE 'Yes', NORMAL WARRANTY '5', and MIN '5'. A search bar is located above the table, containing the text 'New SubType' and a search icon. The search bar is highlighted with a yellow circle.

13 Click this icon.

The screenshot shows the 'Asset Sub Type Configuration' page in the micadpro application. The page has a blue sidebar on the left with 'Asset Register' and 'Configuration' options. The main content area has a header with the micadpro logo and 'Current Application Asset'. Below the header is a table with columns: ID, DETAILS, ASSET TYPE, LIFE, and NORMAL WARRANTY. The table contains one row with ID 626, DETAILS 'New SubType', ASSET TYPE 'Fire Doors', LIFE 'Yes', and NORMAL WARRANTY '5'. A search bar is located above the table, containing the text 'New SubType' and a search icon. The search icon is highlighted with a yellow circle.

14

You can also toggle search via the life toggle; it has three positions: it is defaulted to 'All' that can be changed to 'Yes'

micad pro lan Johnson Admin [devalpha]

Sub Type Configuration + Create Sub Type

.S	ASSET TYPE	LIFE	NORMAL WARRANTY	MIN LIFE	MAX LIFE	STANDARD LIFE
ch	<input type="text" value="Search"/>	<input checked="" type="radio"/>				
CITATION TROLLEY	Fire Door - External	<input checked="" type="radio"/>	0	0	0	0
E ANAESTHETIC EQUIP	Fire Doors	No	0	0	0	0
L ANAESTHETIC EQUIP	Fire Door - External	No	0	0	0	0
S MACHINE	Fire Door - External	No	0	0	0	0
ATOR	Fire Door - External	No	0	0	0	0
IE SECONDARIES	Fire Alarms - Associated Equipment - Healthcare	No	0	0	0	0
INARY FUNCTION REC	Fire Door - External	No	0	0	0	0
THETICS GEN EQUIP	Fire Alarms - Associated Equipment - Healthcare	No	0	0	0	0
CITATOR RESPIRATRY	Fire Door - External	No	0	0	0	0
. ALARM PNEUMATIC	Fire Doors	Yes	14	17	12	13
-ST		No	0	0	0	0
-ST		No	0	0	0	0
ibType	Fire Doors	Yes	5	5	5	5

15


Clicking again will set it to No.


micad pro lan Johnson Admin [devalpha]

Sub Type Configuration + Create Sub Type

.S	ASSET TYPE	LIFE	NORMAL WARRANTY	MIN LIFE	MAX LIFE	STANDARD LIFE
ch	<input type="text" value="Search"/>	<input type="radio"/>				
. ALARM PNEUMATIC	Fire Doors	Yes	14	17	12	13
ibType	Fire Doors	Yes	5	5	5	5

16 or back to 'All.'



Ian Johnson
Admin [devalpha] 

Sub Type Configuration + Create Sub Type

S	ASSET TYPE	LIFE	NORMAL WARRANTY	MIN LIFE	MAX LIFE	STANDARD LIFE
ch	<input type="text" value="Search"/>					
CITATION TROLLEY	Fire Door - External	No	0	0	0	0
E ANAESTHETIC EQUIP	Fire Doors	No	0	0	0	0
L ANAESTHETIC EQUIP	Fire Door - External	No	0	0	0	0
S MACHINE	Fire Door - External	No	0	0	0	0
ATOR	Fire Door - External	No	0	0	0	0
IE SECONDARIES	Fire Alarms - Associated Equipment - Healthcare	No	0	0	0	0
INARY FUNCTION REC	Fire Door - External	No	0	0	0	0
THETICS GEN EQUIP	Fire Alarms - Associated Equipment - Healthcare	No	0	0	0	0
CITATOR RESPIRATRY	Fire Door - External	No	0	0	0	0
-ST		No	0	0	0	0
-ST		No	0	0	0	0

Edit Asset Sub Types

17 To edit a subtype, double-click on it.

⋮	609	MOBILE ANAESTHETIC EQUIP	Fire Doors	No	0	0
⋮	610	DENTAL ANAESTHETIC EQUIP	Fire Door - External	No	0	0
⋮	611	BOYLES MACHINE	Fire Door - External	No	0	0
⋮	612	INCUBATOR	Fire Door - External	No	0	0
⋮	613	PIPELINE SECONDARIES	Fire Alarms - Associated Equipment - Healthcare	No	0	0
⋮	614	PULMONARY FUNCTION REC	Fire Door - External	No	0	0
⋮	615	ANAESTHETICS GEN EQUIP	Fire Alarms - Associated Equipment - Healthcare	No	0	0
⋮	616	RESUSCITATOR RESPIRATRY	Fire Door - External	No	0	0
⋮	617	VENTIL. ALARM PNEUMATIC	Fire Doors	Yes	14	17
⋮	624	TestAV-ST		No	0	0
⋮	625	TestAV-ST		No	0	0
⋮	626	New SubType	Fire Doors	Yes	5	5

Rows per page:

18 Make your changes and click 'Save.'

The screenshot shows a modal dialog titled "Edit Sub Type" with a close button (X) in the top right. The dialog contains the following fields:

- Details ***: A text input field labeled "New SubType" with a clear (X) button.
- Normal Warranty**: A numeric input field with the value "5" and a clear (X) button.
- Asset Type**: A dropdown menu showing "Fire Doors" with a clear (X) button and a dropdown arrow.
- Life**: A toggle switch that is currently turned on.
- Min Life**: A numeric input field with the value "5" and a clear (X) button.
- Max Life**: A numeric input field with the value "5" and a clear (X) button.
- Standard Life**: A numeric input field with the value "5" and a clear (X) button.

At the bottom of the dialog are two buttons: "DELETE" and "SAVE". The "SAVE" button is highlighted with a yellow circle. The background shows a table with columns for asset details and numerical values. At the bottom right of the table, it says "Rows per page: 25 | 1 - 13 of 13 | 1".

19 Alternatively, click on the three dots and click 'Edit.'

The screenshot shows a table with the following data:

609	MOBILE ANAESTHETIC EQUIP	Fire Doors	No	0
610	DENTAL ANAESTHETIC EQUIP	Fire Door - External	No	0
611	BOYLES MACHINE	Fire Door - External	No	0
612	INCUBATOR	Fire Door - External	No	0
613	PIPELINE SECONDARIES	Fire Alarms - Associated Equipment - Healthcare	No	0
614	PULMONARY FUNCTION REC	Fire Door - External	No	0
615	ANAESTHETICS GEN EQUIP	Fire Alarms - Associated Equipment - Healthcare	No	0
616	RESUSCITATOR RESPIRATRY	Fire Door - External	No	0
617	VENTIL. ALARM PNEUMATIC	Fire Doors	Yes	14
624	TestAV-ST		No	0
625	TestAV-ST		No	0
616	New SubType	Fire Doors	Yes	5

A vertical blue sidebar on the left contains a "Help" icon and a back arrow. A yellow circle highlights the three-dot menu icon for the row "616 New SubType". At the bottom right of the table, it says "Rows".

20 Click here.

⋮	609	MOBILE ANAESTHETIC EQUIP	Fire Doors	No	0
⋮	610	DENTAL ANAESTHETIC EQUIP	Fire Door - External	No	0
⋮	611	BOYLES MACHINE	Fire Door - External	No	0
⋮	612	INCUBATOR	Fire Door - External	No	0
⋮	613	PIPELINE SECONDARIES	Fire Alarms - Associated Equipment - Healthcare	No	0
⋮	614	PULMONARY FUNCTION REC	Fire Door - External	No	0
⋮	615	ANAESTHETICS GEN EQUIP	Fire Alarms - Associated Equipment - Healthcare	No	0
⋮	616	RESUSCITATOR RESPIRATRY	Fire Door - External	No	0
⋮	617	VENTIL. ALARM PNEUMATIC	Fire Doors	Yes	14
⋮	624	TestAV-ST		No	0
⋮	625	TestAV-ST		No	0
⋮	626	New SubType	Fire Doors	Yes	5

Select
Edit
Delete

Help

<<

Row

Deleting Asset Sub Types

21 To delete a subtype, double-click on it.

⋮	609	MOBILE ANAESTHETIC EQUIP	Fire Doors	No	0	0
⋮	610	DENTAL ANAESTHETIC EQUIP	Fire Door - External	No	0	0
⋮	611	BOYLES MACHINE	Fire Door - External	No	0	0
⋮	612	INCUBATOR	Fire Door - External	No	0	0
⋮	613	PIPELINE SECONDARIES	Fire Alarms - Associated Equipment - Healthcare	No	0	0
⋮	614	PULMONARY FUNCTION REC	Fire Door - External	No	0	0
⋮	615	ANAESTHETICS GEN EQUIP	Fire Alarms - Associated Equipment - Healthcare	No	0	0
⋮	616	RESUSCITATOR RESPIRATRY	Fire Door - External	No	0	0
⋮	617	VENTIL. ALARM PNEUMATIC	Fire Doors	Yes	14	17
⋮	624	TestAV-ST		No	0	0
⋮	625	TestAV-ST		No	0	0
⋮	626	New SubType	Fire Doors	Yes	5	5

Rows per page: 2

22 Click 'Delete.'

⋮	609	MOBILE ANAESTHETIC EQUIP	Fire Doors	No	0
⋮	610	DENTAL ANAESTHETIC EQUIP			0
⋮	611	BOYLES MACHINE			0
⋮	612	INCUBATOR			0
⋮	613	PIPELINE SECONDARIES			0
⋮	614	PULMONARY FUNCTION REC			0
⋮	615	ANAESTHETICS GEN EQUIP			0
⋮	616	RESUSCITATOR RESPIRATRY			0
⋮	617	VENTIL. ALARM PNEUMATIC			14
⋮	624	TestAV-ST			0
⋮	625	TestAV-ST			0
⋮	626	New SubType			5

Edit Sub Type

Details *
New SubType

Asset Type
Fire Doors

Life

Normal Warranty
5

Min Life
5

Max Life
5

Standard Life
5

DELETE SAVE

23

click 'OK' to confirm.

... CITATION TROLLEY	Fire Door - External	No	0	0	0	0
... ANAESTHETIC EQUIP	Fire Doors	No	0	0	0	0
... ANAESTHETIC EQUIP	Fire Door - External	No	0	0	0	0
... MACHINE	Fire Door - External	No	0	0	0	0
... INCUBATOR	Fire Door - External	No	0	0	0	0
... PIPELINE SECONDARIES		No	0	0	0	0
... PULMONARY FUNCTION REC		No	0	0	0	0
... ANAESTHETICS GEN EQUIP		No	0	0	0	0
... RESUSCITATOR RESPIRATORY		No	0	0	0	0
... VENTIL. ALARM PNEUMATIC		Yes	14	17	12	13
... TEST AV-ST		No	0	0	0	0
... TEST AV-ST		No	0	0	0	0
SubType	Fire Doors	Yes	5	5	5	5

Confirm

Are you sure you want to delete the selected asset sub type(s)?

CANCEL OK

24

Alternatively click on the three dots.

⋮	609	MOBILE ANAESTHETIC EQUIP	Fire Doors	No	0
⋮	610	DENTAL ANAESTHETIC EQUIP	Fire Door - External	No	0
⋮	611	BOYLES MACHINE	Fire Door - External	No	0
⋮	612	INCUBATOR	Fire Door - External	No	0
⋮	613	PIPELINE SECONDARIES	Fire Alarms - Associated Equipment - Healthcare	No	0
⋮	614	PULMONARY FUNCTION REC	Fire Door - External	No	0
⋮	615	ANAESTHETICS GEN EQUIP	Fire Alarms - Associated Equipment - Healthcare	No	0
⋮	616	RESUSCITATOR RESPIRATORY	Fire Door - External	No	0
⋮	617	VENTIL. ALARM PNEUMATIC	Fire Doors	Yes	14
⋮	624	TestAV-ST		No	0
⋮	625	TestAV-ST		No	0
⋮	626	New SubType	Fire Doors	Yes	5

Help

<<

Row

25 Click here.

609	MOBILE ANAESTHETIC EQUIP	Fire Doors	No	0
610	DENTAL ANAESTHETIC EQUIP	Fire Door - External	No	0
611	BOYLES MACHINE	Fire Door - External	No	0
612	INCUBATOR	Fire Door - External	No	0
613	PIPELINE SECONDARIES	Fire Alarms - Associated Equipment - Healthcare	No	0
614	PULMONARY FUNCTION REC	Fire Door - External	No	0
615	ANAESTHETICS GEN EQUIP	Fire Alarms - Associated Equipment - Healthcare	No	0
616	RESUSCITATOR RESPIRATRY	Fire Door - External	No	0
617	VENTIL. ALARM PNEUMATIC	Fire Doors	Yes	14
624	TestAV-ST		No	0
625	TestAV-ST		No	0
626	New SubType	Fire Doors	Yes	5

Select
Edit
Delete

Help

Ro

26 Choose 'OK' to confirm.

CITATION TROLLEY	Fire Door - External	No	0	0	0	0
E ANAESTHETIC EQUIP	Fire Doors	No	0	0	0	0
L ANAESTHETIC EQUIP	Fire Door - External	No	0	0	0	0
S MACHINE	Fire Door - External	No	0	0	0	0
ATOR	Fire Door - External	No	0	0	0	0
E SECONDARIES		No	0	0	0	0
NARY FUNCTION REC		No	0	0	0	0
THETICS GEN EQUIP		No	0	0	0	0
CITATOR RESPIRATRY		No	0	0	0	0
.ALARM PNEUMATIC		es	14	17	12	13
ST		No	0	0	0	0
ST		No	0	0	0	0
bType	Fire Doors	Yes	5	5	5	5

Confirm

Are you sure you want to delete the selected asset sub type(s)?

CANCEL OK

27

To select multiple for deletion, put the grid into selection mode by clicking the three dots.

Asset Register
Configuration

Current Application: Asset

micadpro

Asset Sub Type Configuration

ID	DETAILS	ASSET TYPE	LIFE	NORMAL WARRANTY
608	RESUSCITATION TROLLEY	Fire Door - External	No	0
609	MOBILE ANAESTHETIC EQUIP	Fire Doors	No	0
610	DENTAL ANAESTHETIC EQUIP	Fire Door - External	No	0
611	BOYLES MACHINE	Fire Door - External	No	0
612	INCUBATOR	Fire Door - External	No	0
613	PIPELINE SECONDARIES	Fire Alarms - Associated Equipment - Healthcare	No	0
614	PULMONARY FUNCTION REC	Fire Door - External	No	0
615	ANAESTHETICS GEN EQUIP	Fire Alarms - Associated Equipment - Healthcare	No	0
616	RESUSCITATOR RESPIRATORY	Fire Door - External	No	0
617	VENTIL. ALARM PNEUMATIC	Fire Doors	Yes	14
624	TestAV-ST		No	0
625	TestAV-ST		No	0
626	New SubType	Fire Doors	Yes	5

28

choosing 'Select'

Asset Register
Configuration

Current Application: Asset

micadpro

Asset Sub Type Configuration

ID	DETAILS	ASSET TYPE	LIFE	NORMAL WARRANTY
608	RESUSCITATION TROLLEY	Fire Door - External	No	0
609	MOBILE ANAESTHETIC EQUIP	Fire Doors	No	0
610	DENTAL ANAESTHETIC EQUIP	Fire Door - External	No	0
611	BOYLES MACHINE	Fire Door - External	No	0
612	INCUBATOR	Fire Door - External	No	0
613	PIPELINE SECONDARIES	Fire Alarms - Associated Equipment - Healthcare	No	0
614	PULMONARY FUNCTION REC	Fire Door - External	No	0
615	ANAESTHETICS GEN EQUIP	Fire Alarms - Associated Equipment - Healthcare	No	0
616	RESUSCITATOR RESPIRATORY	Fire Door - External	No	0
617	VENTIL. ALARM PNEUMATIC	Fire Doors	Yes	14
624	TestAV-ST		No	0
625	TestAV-ST		No	0
626	New SubType	Fire Doors	Yes	5

- Select
- Edit
- Delete

29 Make your selection and click delete.

<input type="checkbox"/>	609	MOBILE ANAESTHETIC EQUIP	Fire Doors	No	0
<input type="checkbox"/>	610	DENTAL ANAESTHETIC EQUIP	Fire Door - External	No	0
<input type="checkbox"/>	611	BOYLES MACHINE	Fire Door - External	No	0
<input checked="" type="checkbox"/>	612	INCUBATOR	Fire Door - External	No	0
<input checked="" type="checkbox"/>	613	PIPELINE SECONDARIES	Fire Alarms - Associated Equipment - Healthcare	No	0
<input checked="" type="checkbox"/>	614	PULMONARY FUNCTION REC	Fire Door - External	No	0
<input type="checkbox"/>	615	ANAESTHETICS GEN EQUIP	Fire Alarms - Associated Equipment - Healthcare	No	0
<input type="checkbox"/>	616	RESUSCITATOR RESPIRATRY	Fire Door - External	No	0
<input type="checkbox"/>	617	VENTIL. ALARM PNEUMATIC	Fire Doors	Yes	14
<input type="checkbox"/>	624	TestAV-ST		No	0
<input type="checkbox"/>	625	TestAV-ST		No	0
<input type="checkbox"/>	626	New SubType	Fire Doors	Yes	5

Help

Edit Delete

Clear Selection Select All

3 of 13 selected

30 Click OK to confirm.

CITATION TROLLEY	Fire Door - External	No	0	0	0	0
E ANAESTHETIC EQUIP	Fire Doors	No	0	0	0	0
L ANAESTHETIC EQUIP	Fire Door - External	No	0	0	0	0
S MACHINE	Fire Door - External	No	0	0	0	0
ATOR	Fire Door - External	No	0	0	0	0
E SECONDARIES		No	0	0	0	0
NARY FUNCTION REC		No	0	0	0	0
THETICS GEN EQUIP		No	0	0	0	0
CITATOR RESPIRATRY		No	0	0	0	0
.ALARM PNEUMATIC		Yes	14	17	12	13
ST		No	0	0	0	0
ST		No	0	0	0	0
bType	Fire Doors	Yes	5	5	5	5

Confirm

Are you sure you want to delete the selected asset sub type(s)?

CANCEL OK